


# PIPETTE CALIBRATION TREND ANALYSIS - ACCURACY % vs CALIBRATION

Date: 4/28/2009 Time: 2:40:30 PM  
 Device ID: 1358404954  
 Description: Gilson Pipetman P-100, variable, 100ul, 1ch  
 Method: Control Calibrations  
 Test Plan: 100 ul, variable

Customer: ABC Laboratories  
 Contact: Susan Smith  
 Location: Lab room 107  
 Address: 555 Aliquot Lane  
 Savannah



All Samples View

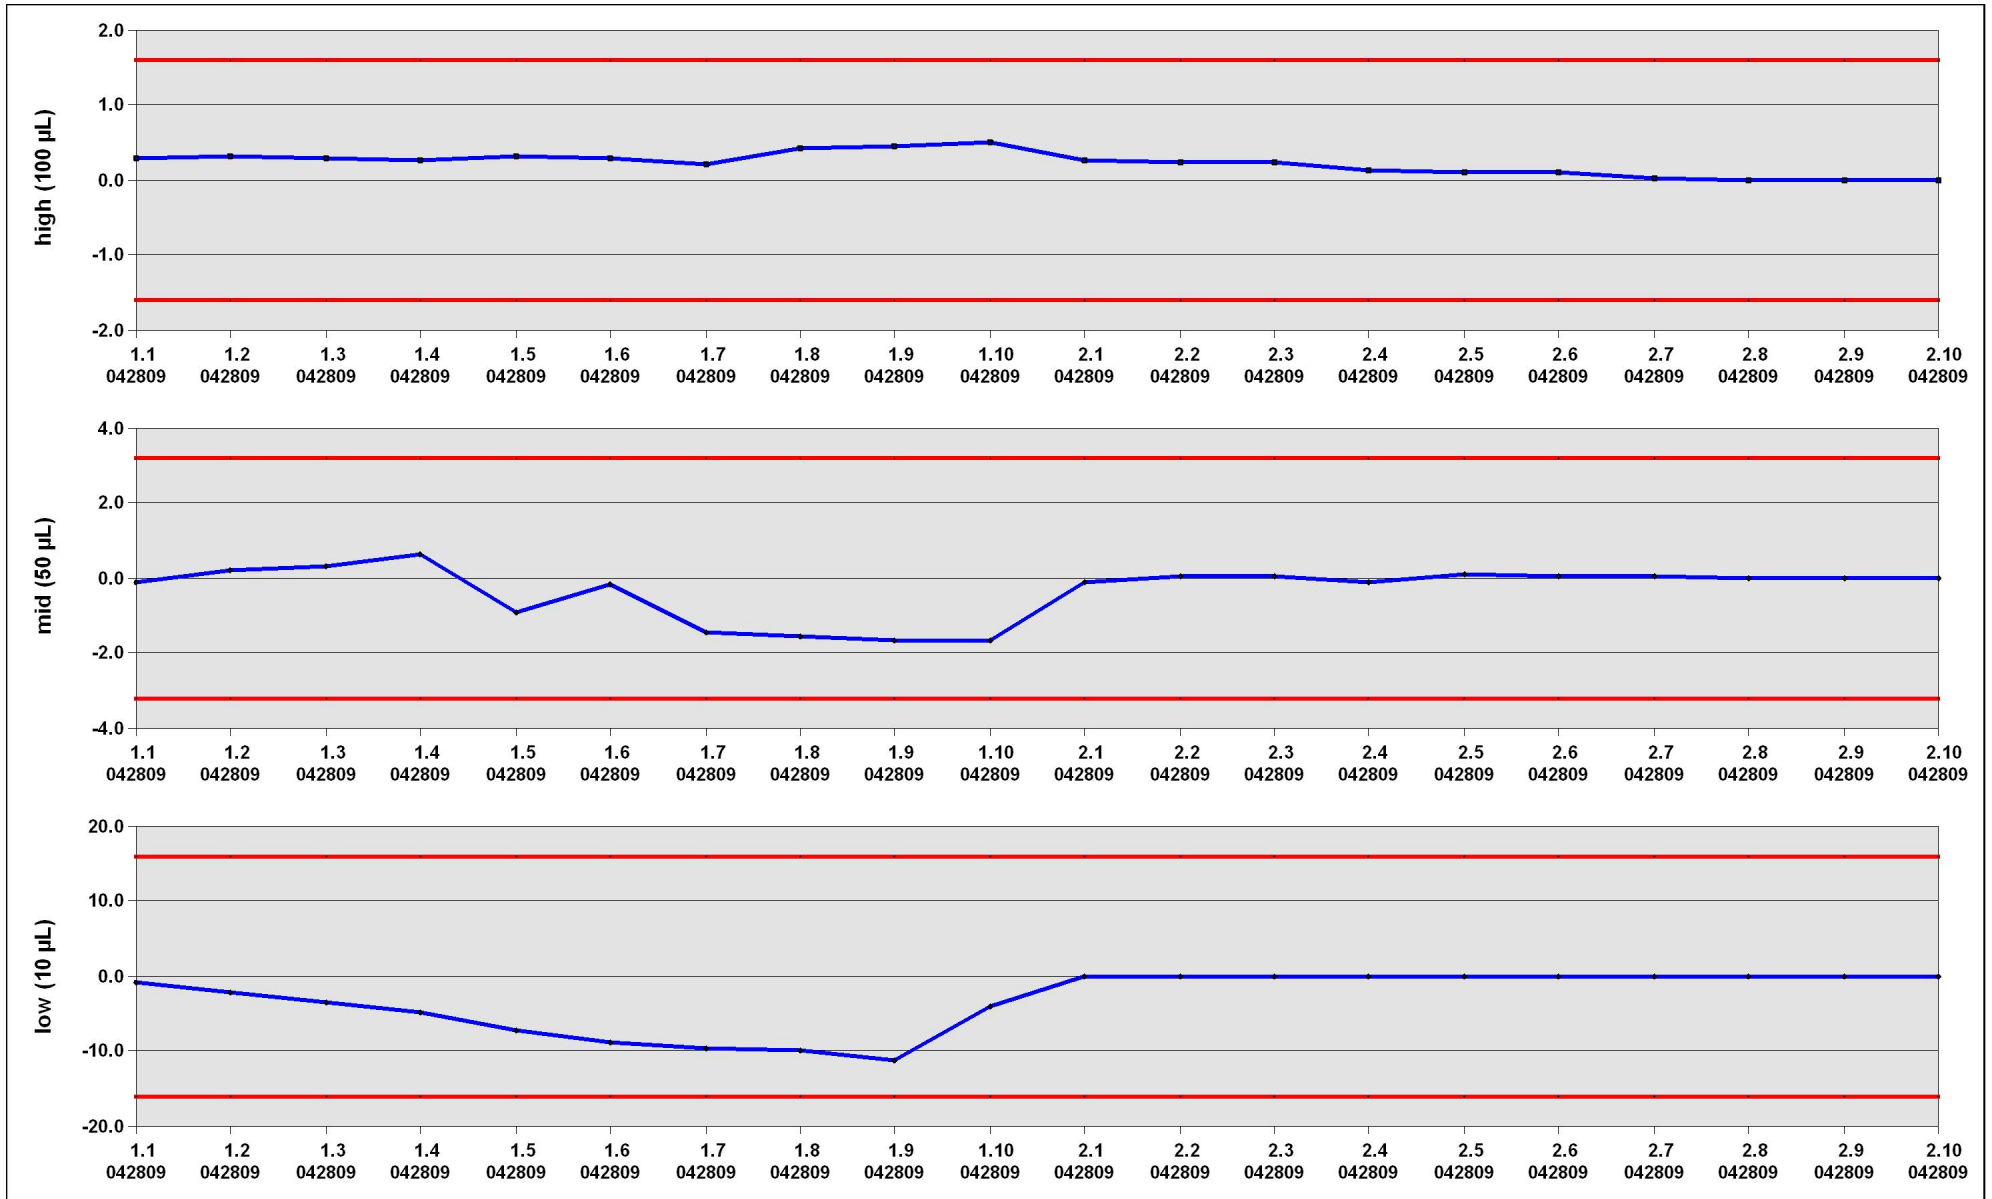

Signature: \_\_\_\_\_

Date: \_\_\_\_\_